



The Intelligent Analyzer.

Assuring quality before, during and after sample analysis—for improved patient care.



Improving patient Now that's intelligent

With the GEM Premier 5000 system:*

- ▶ iQM2 provides **real-time assurance**
- ▶ All-in-one, multi-use GEM PAK offers **advanced simplicity**
- ▶ GEMweb® Plus 500 Custom Connectivity allows **complete management**

In the lab and at the point of care

*Not available in all countries.

care and efficiency. ent.

Real-time quality assurance, everywhere

New iQM2 with IntraSpect™ technology provides intelligent analyzing—automated quality assurance with every sample, continuously and in real time, unlike traditional (auto or manual) quality control (QC) offerings.

Real-time detection

iQM2 performs continuous checks—**before, during** and **after** every sample.

Immediate, automatic correction

Automatic documentation

Advanced simplicity, anywhere

- Self-contained GEM PAKs
- Available in different menu and test-volume configurations
- Allow ultimate flexibility for the needs of specific units (e.g., ICU, NICU, CVOR, ED)
- **31-days[†]** use-life and **require no refrigeration**


[†]21-day onboard use-life for 600-test PAK.



30 different GEM PAK configurations available.


iQM2: Real-time detection, correction and documentation

- Error detection reduced from hours to minutes
- A complete picture of quality for each and every sample
- Designed to mitigate risks in all phases of testing, from pre-analytical through post-analytical

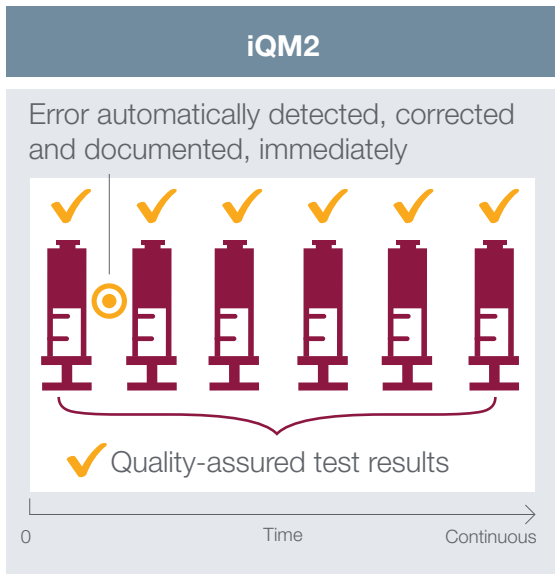

iQM2 assures quality continuously

VS.

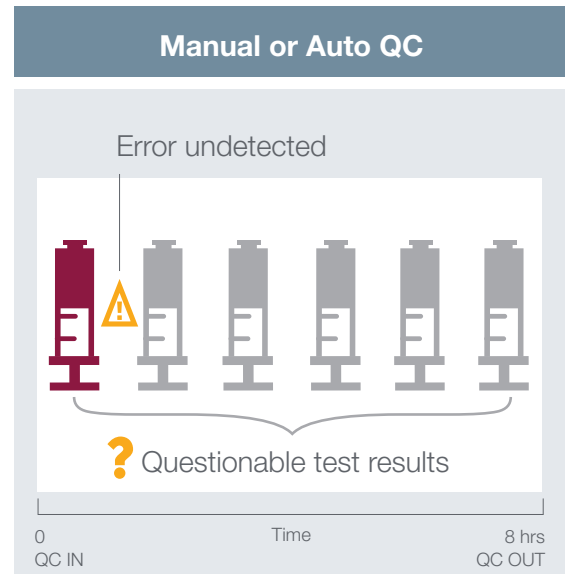

All results from 8-hour period require review

Reduces error detection time from hours to minutes^{1,2} and detects transient sample-specific errors that traditional QC methods miss.

	pH	pO ₂	pCO ₂	Na ⁺	K ⁺	Ca ⁺⁺	Cl ⁻	Glu	Lac	Hct	tHb	tBili
iQM2* (mins)	2	2	2	4.1	2	2	2	16.8	2	2	2	2
Traditional QC (manual or auto)	← ≥8 hrs →											

Statistical presentation of an average error detection time with 95% confidence.

Automated, real-time assurance helps ensure accurate results with every sample

- Provides caregivers more time at the bedside
- Fast and quality-assured test results allow for immediate patient management decisions
- Eliminates unnecessary retesting, for higher patient and staff satisfaction

*Together with James Westgard, PhD, Instrumentation Laboratory established the methodology for optimizing high probability of error detection and low probability of false rejection of drift limits. Method performance, in terms of mean and Standard Deviation, of measured Process Control Solutions (PCS) values were obtained from the data of 276 GEM PAK cartridges used in Proof-of-Performance and external studies for the GEM Premier 5000 analyzer.

How is it possible?

- **iQM2 functions within a stable, closed analytical system**
 - Eliminates outside variables
 - Ensures errors are known and limited
- **Identifies errors through patented Pattern Recognition software**
 - Pattern Recognition is at the heart of iQM2 functionality
 - Possible only with a stable, closed analytical system to which the user cannot introduce change
- **Analyzes 5 levels of PCSs continuously to confirm sensor and PAK performance**

All-in-one, multi-use GEM PAK



Continuous monitoring through 5 PCSs at Medical Decision Levels (MDL)

- PCSs are traceable to Clinical & Laboratory Standards Institute (CLSI) and National Institute of Standards and Technology (NIST) primary standards
- Each PCS follows the same pathway as a patient sample and serves a specific function in the iQM2 process
- Established target values monitor MDLs and ensure accuracy of results
- Monitoring MDLs is essential to ensure accuracy in clinical decisions, particularly in critically ill patients (e.g., lactate MDL align with recommended values for treatment of sepsis)


Only iQM2 assures the integrity of every sample in real time

The only continuous quality management system that checks sample integrity before, during and after every sample analysis.

- Features patented Pattern Recognition technology in a single-cartridge, stable, closed system
- Auto-detects transient errors during sample analysis that other QC methods could miss
- Auto-documents all errors and corrections
- Generates operator- and sample quality-specific reports to help managers proactively support quality improvement initiatives*

*Available through GEMweb Plus 500 Custom Connectivity.


Only iQM2 conducts a continuous cycle of 5 quality checks—more than any other blood gas system

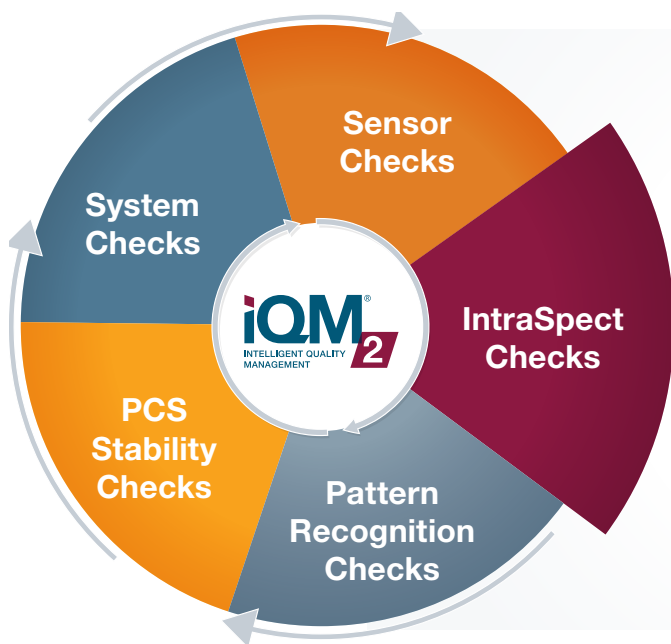

Only iQM2 has IntraSpect technology

Detects sample-specific errors during sample measurement that traditional QC methods could miss (e.g., micro-clots, micro-bubbles, interferences). If missed, these errors may affect current or future sample integrity.

Quality management with every second of analysis: iQM2 in real time

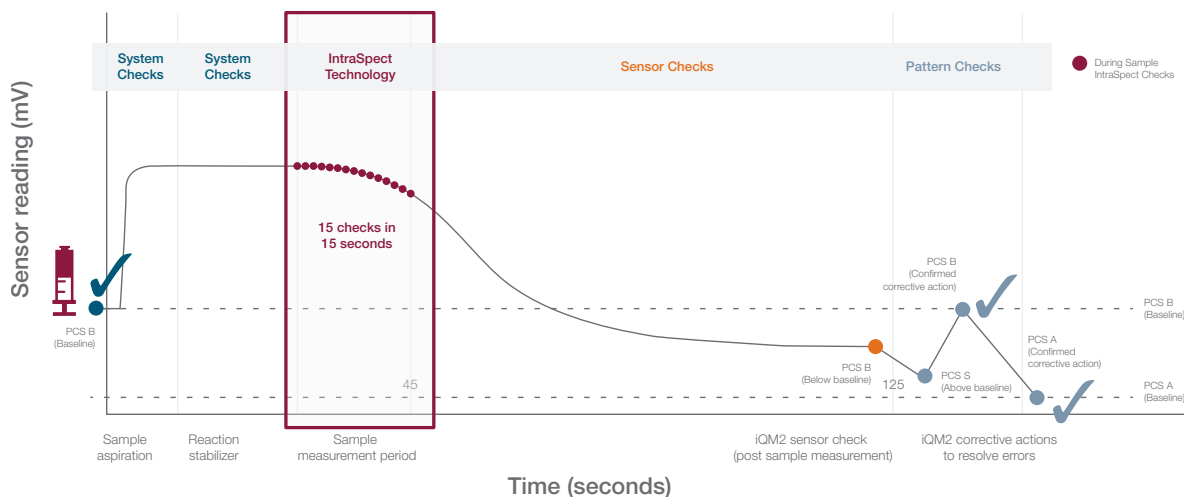


Only iQM2 offers complete automation of sample quality management

Performs auto-detection, -correction and -documentation, plus sample-handling reports, tailored training programs and certification—uniquely improve quality and management.*


*Reports available through GEMweb Plus 500 Custom Connectivity.




1 Real-time error detection

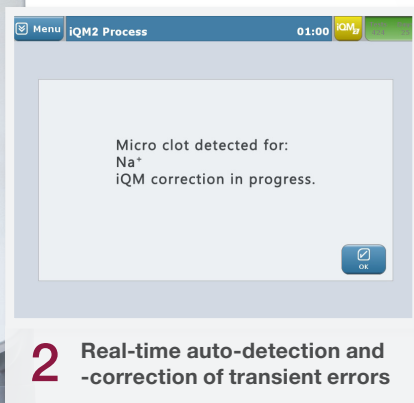

2 Real-time auto-detection and -correction of transient errors

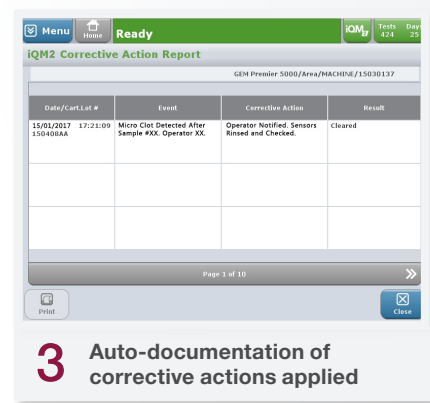

3 Auto-documentation of corrective actions applied

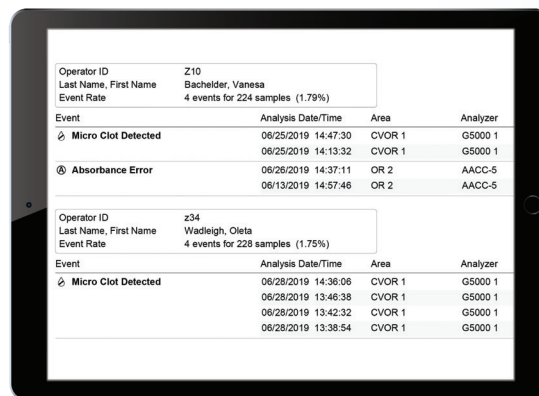

Sample handling reports traceable to operator or clinical setting

(from GEMweb Plus 500 Custom Connectivity)

FDA-cleared technology

“iQM2 manages the quality control process, replacing external quality control.”


– US Food and Drug Administration

GEM PAK: Advanced simplicity at every point of care

Automates the most labor- and skill-intensive processes.

- Zero maintenance—just replace the disposable, all-in-one, multi-use PAK monthly; no additional cartridge-handling required**
 - Includes all testing components: sensors, CO-Ox optical cell, lysing solution, PCSs, tubing, waste bag and sampler
 - Only 1 PAK to inventory and manage
 - No hands-on troubleshooting or corrective actions required
- Ensures patient and operator safety**
 - All components are self-contained, limiting operator biohazard exposure
 - No blood enters the analyzer, limiting infection exposure for patient and operator
- Ultimate simplicity—no special requirements**
 - Easy front-loading
 - Room-temperature storage; no refrigeration required
 - Replaced every 31 days—only 12 PAKs per year*
 - Ideal for high- and low-volume testing

Annual Cartridge Utilization Comparison†

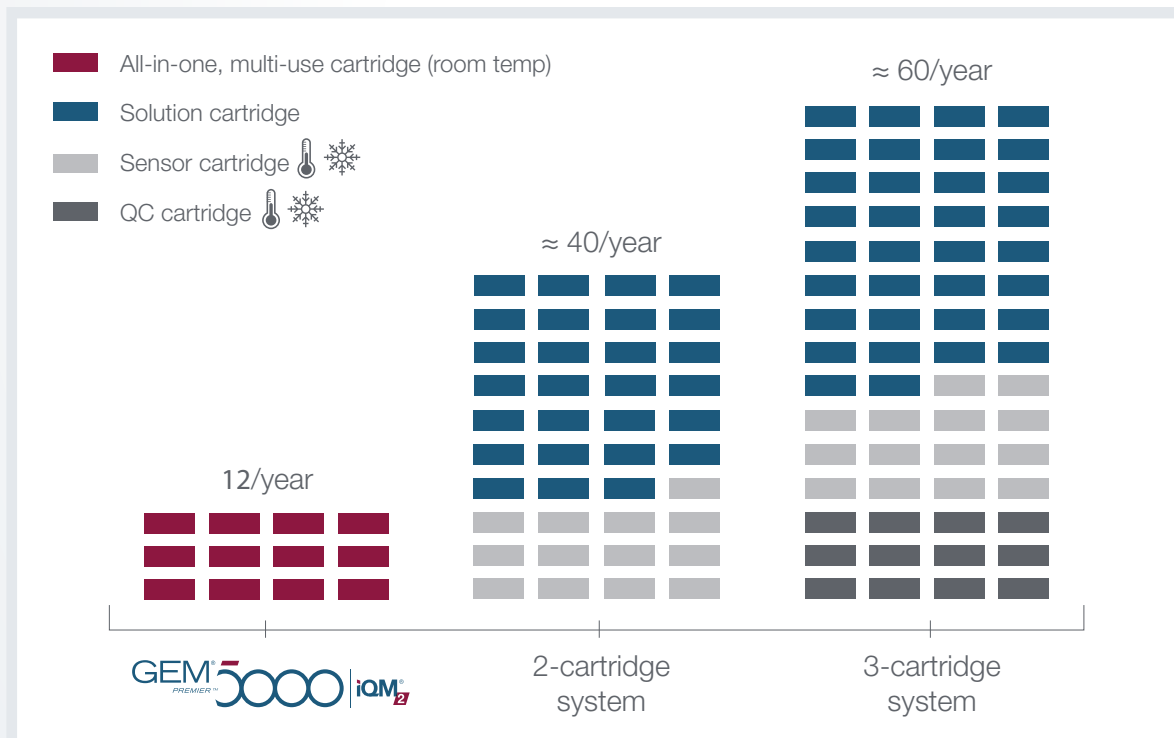

*Assumes constant test volume of 450 samples/month or less.

†Based on 1 analyzer with annual sample volume ≈ 4,800 and QC requirement of 3 times/day. Data on file, IL.

‡* Requires refrigeration.



GEM PAK contains all analytical and quality control components.

Management and compliance simplified

GEMweb Plus 500 Custom Connectivity provides customizable connectivity and automated functionality for complete control of analyzers, operators and data oversight.



Simple, intuitive dashboard, accessible from any analyzer, PC or tablet.

Simplify POCT

- Simple web access from any browser
- Optimized interface for access from analyzer and tablet devices
- Easy at-a-glance dashboard
- Real-time remote management of analyzer configuration without testing interruption
- Total automated management of operators with multi-level authorization and traceability of users, actions and competence

Centralize POCT

- Single unified database to access patient samples and historical results
- Data connection to iQM on GEM Premier 3500/4000 and GEM Premier ChemSTAT™ systems
- Data connection to iQM2 on GEM Premier 5000 systems
- Customizable to multiple connection types, including patient monitors, HIS/LIS and ADT
- Open connectivity, including select non-IL analyzers[†]

What's different about the GEM Premier 5000 system?

Advanced Simplicity *outside*



Custom Quick Start sampling

Programmed shortcuts expedite testing

Illuminated sampling area

Ensures proper capillary or syringe insertion

Universal sampling

Accepts tubes, syringes or capillaries

Smartcolor status bar

Analyzer status at a glance

Fast time to result

45 seconds including quality checks

i-button for iQM2

Conveys real-time iQM2 status

Motion-detection barcode reader

Enables one-hand use

Real-Time Assurance

inside

iQM² with IntraSpect technology

Provides a complete picture of quality for each sample

AutoPAK Validation

Standardizes time-to-ready state



Improve patient care *and* efficiency

Improved patient care

- Rapid, quality-assured test results with every sample, not just every 8 hours
- Identifies and reduces risks associated with testing processes before, during and after every sample
- Prevents the reporting of erroneous results
- Enables staff to spend less time maintaining/troubleshooting and more time at the patient's bedside



Ask your IL representative for a customized time, resource and savings calculation.

Improved efficiency

- Automates analyzer and operator management
- Manages quality in self-contained GEM PAKs
- Eliminates outside variability
- Eliminates maintenance
- Menu- and volume-specific GEM PAKs allow customization tailored to unit needs
- Allows system-wide control from any analyzer or PC
- Keeps documentation just a click away

A complete solution for improved patient care and efficiency.



GEM[®] 5000
PREMIER™

iQM[®]
2

GEMweb[®] Plus
CUSTOM CONNECTIVITY

Technical Specifications

Quantitative Measured Analytes

Analyte	Unit
pH	n/a
pCO ₂	mmHg
pO ₂	mmHg
Na ⁺	mmol/L
K ⁺	mmol/L
Ca ⁺⁺	mmol/L
Cl ⁻	mmol/L
Glu	mg/dL
Lac	mmol/L
Hct	%
tHb	g/dL
O ₂ Hb	%
COHb	%
MetHb	%
HHb	%
tBili	mg/dL
sO ₂ *	%

*sO₂ = O₂Hb/O₂Hb+HHb.

Derived (Calculated) Parameters

BE(B)	pAO ₂	O ₂ ct	RI
BE(ecf)	CaO ₂	HCO ₃ ⁻ std	CcO ₂
tHb(c)	CvO ₂	TCO ₂	a-vDO ₂
Ca ⁺⁺ (7.4)	p ₅₀	HCO ₃ ⁻ (c)	Q _{sp} /Q _t (est)
Anion gap (AG)	O ₂ cap	A-aDO ₂	Q _{sp} /Q _t
P/F ratio	sO ₂ (c)	paO ₂ /pAO ₂	Hct(c)

Flexible Customization

Test volumes: 75, 150, 300, 450, 600[†]

Menu

Blood Gas, Hct, tHb, O ₂ Hb, HHb, COHb, MetHb, sO ₂ , tBili [†]
Blood Gas, Electrolytes, Hct, tHb, O ₂ Hb, HHb, COHb, MetHb, sO ₂ , tBili [†]
Blood Gas, Electrolytes, Glu, Lac, Hct, tHb, O ₂ Hb, HHb, COHb, MetHb, sO ₂ , tBili [†]

[†] Onboard use-life is 31-days, except 600-test PAK, which is 21-days.

[‡] PAKs available with or without tBili.

Real-time assurance and advanced simplicity. Now that's intelligent.

- Westgard JO, *et al.* Validation of iQM active process control technology. *Point Care*. 2003;2:1-7.
- Toffaletti JG, *et al.* Validation of a quality assessment of blood gas and electrolyte testing. *Clin Chim Acta*. 2007;382:65-70.

Werfen

Corporate Headquarters

Plaza de Europa, 21-23
08908 L'Hospitalet de Llobregat
Barcelona, Spain
+34-93-4010101
werfen.com

Instrumentation Laboratory Headquarters

180 Hartwell Road
Bedford, MA 01730 USA
+1-781-861-0710
instrumentationlaboratory.com

Worldwide Locations

The Americas

Brazil
São Paulo
+55-11-46227878
br.werfen.com

Canada
Richmond Hill, ON
+1-800-552-2025 x6115
instrumentationlaboratory.com

Colombia
Bogotá
+57-15-221-052

Mexico
Mexico City
+52-55-5262-1760
mx.werfen.com

Uruguay
Montevideo
+5982-481-81-33

USA
Bedford, MA
+1-781-861-0710
instrumentationlaboratory.com

Asia-Pacific

Australia
Sydney
+61-02-9098-0200
au.werfen.com

China
Beijing
+86-10-59756055
Hong Kong
+852-2792-7773
Shanghai
+86-21-66308671
cn.werfen.com

India
New Delhi
+91-490-29-550
in.werfen.com

Japan
Tokyo
+81-3-5419-1301
jp.werfen.com

Korea
Seoul
+82-1899-9217
kr.werfen.com

Thailand
Bangkok
+66-271-226-28/9

Europe

Austria
Vienna
+43-1-256-58-000
at.werfen.com

Belgium
Brussels
+32-2-7252052
benelux.werfen.com

Czech Republic
Prague
+420-246-090-931
cz.werfen.com

France
Paris
+33-182-30-86-00
fr.werfen.com

Germany
Munich
+49-89-909070
de.werfen.com

Hungary
Budapest
+36-1-882-73-10
hu.werfen.com

Italy
Milan
+39-02-25221
it.werfen.com

Lithuania
Kaunas
+370-37-313157
lt.werfen.com

The Netherlands
Breda
+31-76-5480100
benelux.werfen.com

Poland
Warsaw
+48-22-336-18-00

Portugal
Lisbon
+351-214247312
pt.werfen.com

Russia
Moscow
+7-499-124-45-59
ru.ilwerfen.com

Spain
Barcelona
+34-902-20-30-90
es.werfen.com

UK
Warrington, England
+44-1925-810141
uk.werfen.com

For all other countries visit
international.werfen.com

The Instrumentation Laboratory logo, GEM, Premier, GEM Premier ChemSTAT, ChemSTAT, GEMweb, iQM, Hemochron, VerifyNow, Avoximeter and ROTEM are trademarks of Instrumentation Laboratory Company and/or one of its subsidiaries or parent companies and may be registered in the United States Patent and Trademark Office and in other jurisdictions. All other product names, company names, marks, logos and symbols are trademarks of their respective owners.

©2020 Instrumentation Laboratory. All rights reserved.

VINGMED
Vingmed AB
Datavägen 9A, Box 576, 175 26 Järfälla
Tel: 08-583 593 00, Fax: 08-585 570 10

Werfen